Data File C:\HPCHEM\1\DATA\N9709231\030B3001.D   Sample Name: 000945172880

Injection Date	: 9/23/97 7:23:45 PM	Seq. Line :	30
Sample Name	: 000945172880	Vial :	30
Acq. Operator	: martinj	Inj :	1
		Inj Volume :	1 µl
Acq. Method	: C:\HPCHEM\1\METHODS\H2O.M		
Last changed	: 9/23/97 11:43:59 AM by martinj		
Analysis Method	: C:\HPCHEM\1\METHODS\NIC.M		
Last changed	: 10/3/97 10:41:00 AM		
	(modified after loading)		

Water Analysis - Routine Nicotine and Water Analysis

FID2 B, (N9709231\030B3001.D)

WINSTON KS SP
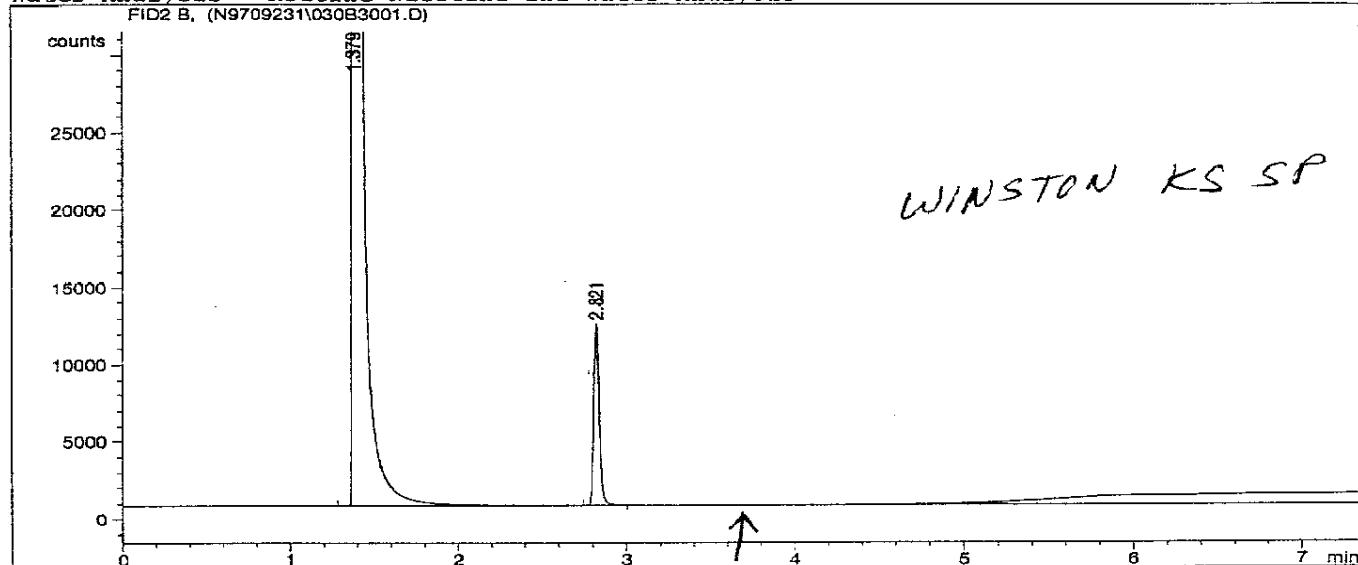
Internal Standard Report (Sample Amount is 0!)

Sorted By	:	Signal
Calib. Data Modified	:	10/3/97 10:35:20 AM
Multiplier	:	1.0000
Dilution	:	1.0000
Uncalibrated Peaks	:	not reported

Sample ISTD Information:

ISTD #	ISTD Amount [mg/cigt]	Name
1	1.00000	Carvone

Signal 1: FID2 B,
    Results obtained with enhanced integrator!

RetTime [min]	Type	Area counts*s	Amt/Area ratio	Amount [mg/cigt]	Grp	Name
2.821	VV T+I	2.68618e4	1.00000	1.00000		Carvone
3.654		-	-	-		Nic

Totals without ISTD(s) :   0.00000

2 Warnings or Errors :

Warning : Time reference compound(s) not found
Warning : Sample amount is zero. Absolute amounts calculated

GC353 10/3/97 10:57:21 AM   Page 1 of 2